



CERTIFICATE OF ANALYSIS FOR
BASE METAL MMCRM OREAS 36

SUMMARY STATISTICS

Constituent	Certified Value	5% window		Relative Standard Deviations			1SD	2SD window		3SD window	
		Low	High	1RSD	2RSD	3RSD		Low	High	Low	High
Mixed Acid Digests (no HF)											
Ag (ppm)	10.17	9.67	10.68	6.23%	12.5%	18.7%	0.63	8.91	11.44	8.27	12.08
As (ppm)	722	686	758	4.45%	8.90%	13.3%	32	658	786	626	819
Cu (ppm)	151	143	158	3.00%	6.00%	8.99%	5	142	160	137	165
Fe (wt.%)	20.68	19.65	21.72	1.80%	3.60%	5.40%	0.37	19.94	21.43	19.57	21.80
Mn (wt.%)	1.08	1.03	1.13	3.11%	6.22%	9.32%	0.03	1.01	1.15	0.98	1.18
Pb (wt.%)	0.579	0.550	0.608	2.84%	5.68%	8.51%	0.016	0.546	0.611	0.529	0.628
Tl (ppm)	~65	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
Zn (wt.%)	4.19	3.98	4.39	1.61%	3.22%	4.83%	0.07	4.05	4.32	3.98	4.39
Peroxide Fusion											
Ag (ppm)	~9.6	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
As (ppm)	699	664	733	7.71%	15.4%	23.1%	54	591	806	537	860
Cu (ppm)	153	145	160	4.42%	8.84%	13.3%	7	139	166	132	173
Fe (wt.%)	21.06	20.01	22.11	4.01%	8.03%	12.0%	0.85	19.37	22.75	18.52	23.60
Mn (wt.%)	1.27	1.21	1.34	2.67%	5.33%	8.00%	0.03	1.20	1.34	1.17	1.37
Pb (wt.%)	0.553	0.525	0.580	2.14%	4.29%	6.43%	0.01	0.529	0.576	0.517	0.588
Tl (ppm)	109	104	115	2.71%	5.42%	8.13%	3	103	115	100	118
Zn (wt.%)	4.22	4.01	4.43	3.15%	6.31%	9.46%	0.13	3.96	4.49	3.82	4.62
Leco											
S (wt.%)	18.81	17.87	19.75	1.15%	2.29%	3.44%	0.22	18.38	19.24	18.16	19.45

Note - intervals may appear asymmetric due to rounding

Prepared by:
Ore Research & Exploration Pty Ltd
June 2008

SOURCE MATERIAL

OREAS certified reference materials (CRMs) are intended to provide a low cost method of evaluating and improving the quality of precious and base metal analysis of geological samples. To the analyst they provide an effective means of calibrating analytical equipment, assessing new techniques and routinely monitoring in-house procedures. To the geologist they provide a means of implementing quality control in analytical data sets generated in exploration, from the grass roots level through to prospect evaluation, and in grade control at mining operations.

OREAS 36 is a low grade zinc ore matrix-matched certified reference material (MMCRM) prepared by Ore Research and Exploration. It is one of 3 MMCRM's sourced from the Gamsberg Zn deposit located in the Northern Cape Province of South Africa, approximately 20km west of the Black Mountain mine. Gamsberg is a stratiform base metal Broken Hill Style (BHS) deposit located in the mid-proterozoic Bushmanland Province of the Namaqualand Metamorphic Complex (NMC) of South Africa. The NMC is a highly deformed and metamorphosed supracrustal succession of dominantly pelitic schists and quartzites, deposited on a regionally extensive ± 2000 Ma basement (Rozendal & Stalder, 2001). The stratiform ores have a close spatial and genetic association with metamorphosed chemical sediments including manganiferous iron formations, quartz-garnet rocks (coticules), Ca-Mn marbles and barite (Rozendal & Stalder, 2001).

COMMINUTION AND HOMOGENISATION PROCEDURES

The material was prepared in the following manner:

- a) *drying at 65^o C to constant mass;*
- b) *crushing and screening;*
- b) *preliminary homogenisation;*
- c) *milling to minus 30 microns;*
- d) *final homogenisation;*
- e) *packaging into 10g units under nitrogen and sealed in laminated foil pouches.*

ANALYSIS OF OREAS 36

Ten commercial laboratories participated in the analytical program to characterise Ag, As, Cu, Fe, Mn, Pb, S, Tl and Zn in OREAS 36. The laboratories were requested to analyse all elements by three acid ore grade digest (preferred) or strong aqua regia digestion together with sodium peroxide fusion methods. To evaluate and compensate for the effects of batch-to-batch variation at individual laboratories, samples were submitted to six of the laboratories in three batches of four 10g samples at weekly intervals. The remaining four laboratories completed one round only. Their data has been included in all statistical analysis excluding performance gates, where only the six labs incorporating batch to batch variation have been used (for further discussion see 'Performance Gates').

All results, together with uncorrected means, medians, one sigma standard deviations, relative standard deviations and percent deviation of lab means from the corrected mean of means (PDM³) are presented in the Appendix (Tables A2 to A18). The parameter PDM³ is a measure of laboratory accuracy while the relative standard deviation is an effective measure of analytical precision where homogeneity of the test material has been confirmed (see 'Statement of Homogeneity' and 'Anova' sections). The analytical methods employed by each laboratory are given in the table captions and described in Table A1 of the Appendix.

All ten commercial labs participated in the acid digest work and employed flame AAS, ICP-OES or ICP-MS instrumental finishes. Up to eight of these labs (depending on the analyte) also carried out sodium peroxide fusion ICP-OES/MS analysis to evaluate the presence of an acid insoluble component. Sulphur was determined via Leco by nine labs with the remaining lab employing aqua regia digest with an ICP-OES finish. Each of the four samples submitted to each laboratory were taken at regular intervals during packaging of the standard in order to maximise their representation. Comparisons of interlaboratory bias and precision are graphically presented in scatter plots for acid digest Pb and Zn (Figures 1 and 2) together with $\pm 3SD$ (magenta) and $\pm 5\%$ (yellow) control lines and certified value (green line). Accepted individual results are coloured blue and individual and dataset outliers are identified by red and violet, respectively.

STATISTICAL EVALUATION OF ANALYTICAL DATA FOR OREAS 36

Certified Value and Confidence Interval

Each batch of results is treated as a separate data set in testing for outliers. The certified value is determined from the mean of lab means after filtering of individual and batch outliers. It is computed according to the formulae

$$\bar{x}_i = \frac{1}{n_i} \sum_{j=1}^{n_i} x_{ij}$$

$$\bar{x} = \frac{1}{p} \sum_{i=1}^p \bar{x}_i$$

where

- x_{ij} is the j th result reported by laboratory i ;
- p is the number of participating laboratories;
- n_i is the number of results reported by laboratory i ;
- \bar{x}_i is the mean for laboratory i ;
- \bar{x} is the mean of means.

The confidence intervals are obtained by calculation of the variance (\hat{V}) of the consensus value (\hat{x}) (mean of means) and reference to Student's- t distribution with degrees of freedom ($p-1$).

$$\hat{V}(\hat{x}) = \frac{1}{p(p-1)} \sum_{i=1}^p (\bar{x}_i - \bar{x})^2$$

$$\text{Confidence Interval} = \bar{x} \pm t_{1-x/2}(p-1)(\hat{V}(\hat{x}))^{1/2}$$

where

$t_{1-x/2}(p-1)$ is the $1-x/2$ fractile of the t -distribution with $(p-1)$ degrees of freedom.

The distribution of the values is assumed to be symmetrical about the mean in the calculation of the confidence interval.

The test for rejection of individual outliers from each laboratory data set is based on z scores (rejected if $|z_i| > 2.5$) computed from the robust estimators of location and scale, T and S , respectively, according to the formulae

$$S = 1.483 \frac{\text{median}_{j=1, \dots, n} |x_j - \text{median}_{i=1, \dots, n}(x_i)|}{}$$

$$z_i = \frac{x_i - T}{S}$$

where

T is the median value in a data set;

S is the median of all absolute deviations from the sample median multiplied by 1.483, a correction factor to make the estimator consistent with the usual parameter of a normal distribution.

Following identification of z-score outliers a 3SD filter is applied, with those values lying outside this window relegated to outlying status also. In certain instances statistician's prerogative has been employed in discriminating outliers. The test for outlying laboratory batches is also based on z-score discrimination (rejected if $|z_i| > 2.5$) and these batches are deleted from the respective lab mean before calculation of the mean of lab means (Certified Value). All outliers are shown in bold and left justified in the tabulated data of the Appendix and to reiterate, have been omitted in the determination of the certified value.

The magnitude of the confidence interval is inversely proportional to the number of participating laboratories and interlaboratory agreement. It is a measure of the reliability of the certified value, i.e. the narrower the confidence interval the greater the certainty in the certified value.

Fig. 1. Mixed Acid Digest (no HF) results for Zn in OREAS 36

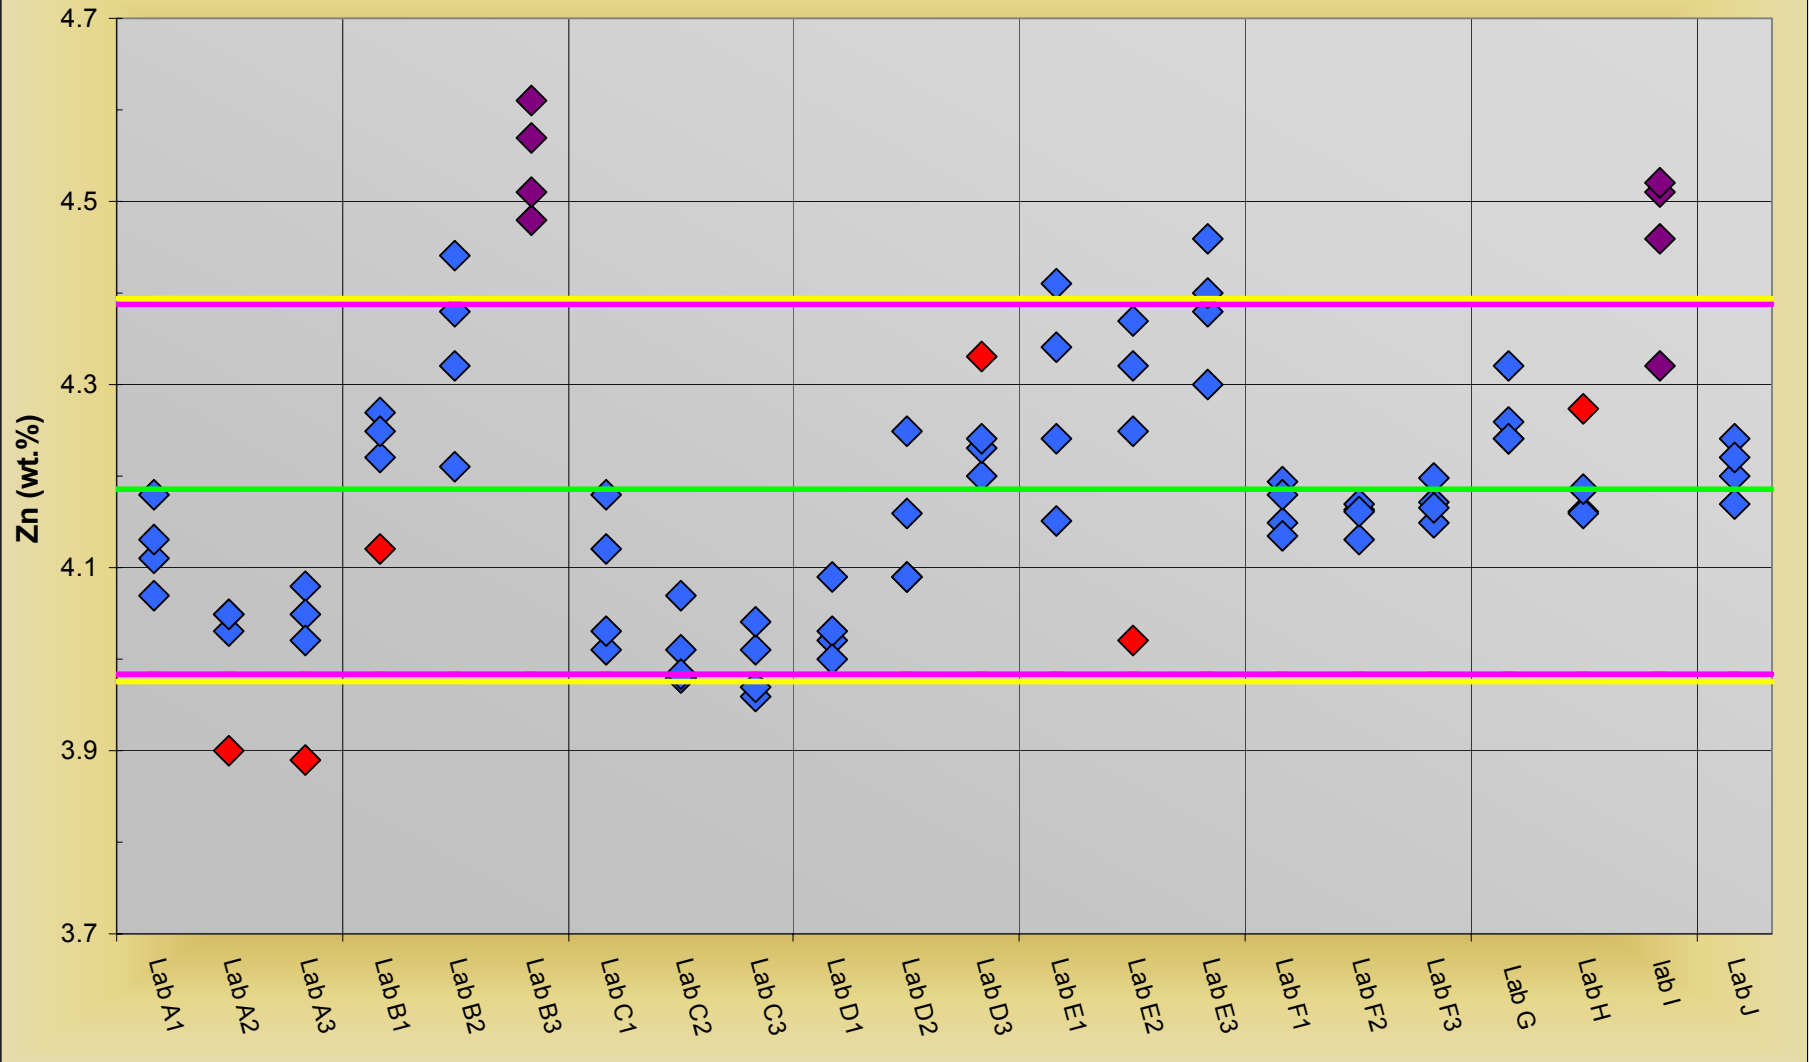


Fig. 2. Mixed Acid Digest (no HF) results for Pb in OREAS 36

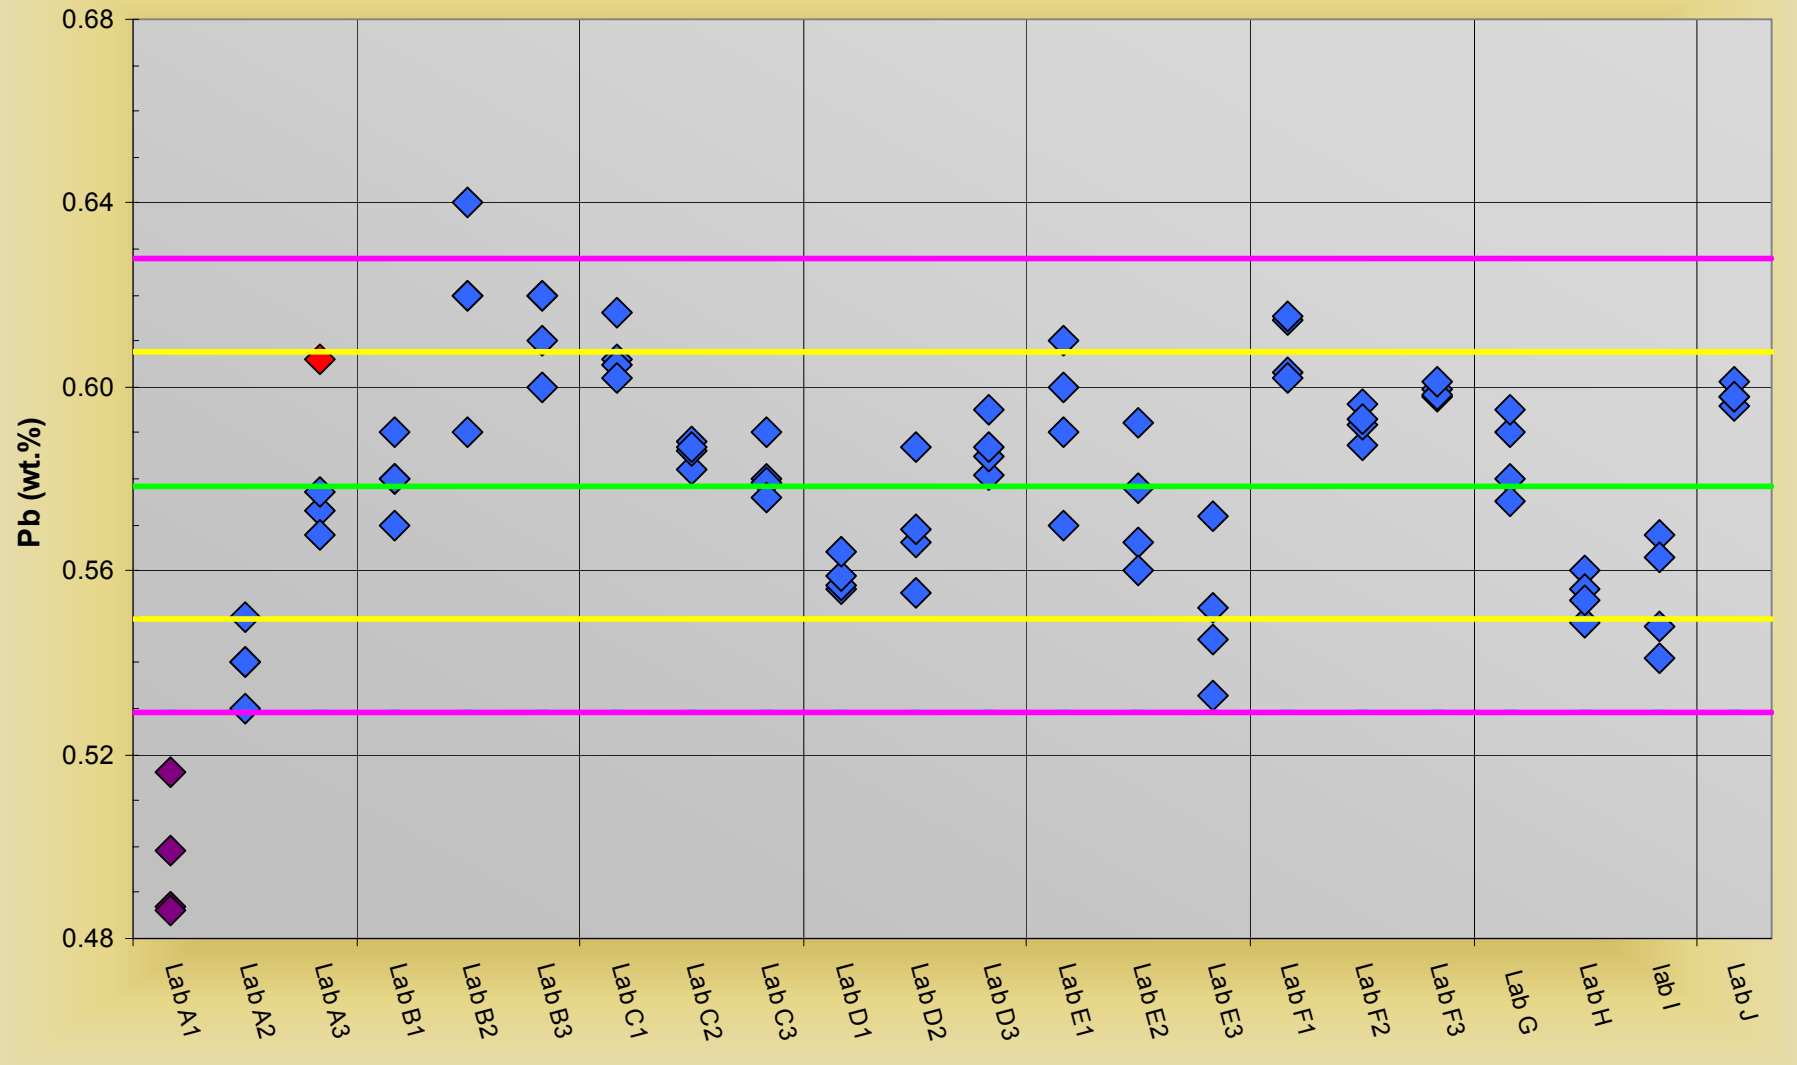


Table 1. Certified Values and 95% Confidence Intervals for OREAS 36.

Constituent	Certified Value	95% Confidence Interval	
		Low	High
Mixed Acid Digests (no HF)			
Silver, Ag (ppm)	10.17	9.77	10.58
Arsenic, As (ppm)	722	707	738
Copper, Cu (ppm)	151	147	155
Iron, Fe (wt.%)	20.68	20.24	21.12
Manganese, Mn (wt.%)	1.08	0.98	1.18
Lead, Pb (wt.%)	0.579	0.564	0.593
Thallium, Tl (ppm)	~65	IND	IND
Zinc, Zn (wt.%)	4.19	4.11	4.26
Peroxide Fusion			
Silver, Ag (ppm)	9.6	8.4	10.9
Arsenic, As (ppm)	699	630	767
Copper, Cu (ppm)	153	150	155
Iron, Fe (wt.%)	21.06	20.35	21.77
Manganese, Mn (wt.%)	1.27	1.24	1.30
Lead, Pb (wt.%)	0.553	0.540	0.565
Thallium, Tl (ppm)	109	97	122
Zinc, Zn (wt.%)	4.22	4.08	4.37
Leco			
Sulphur, S (wt.%)	18.81	18.39	19.23

Note - intervals may appear asymmetric due to rounding

Statement of Homogeneity

The standard deviation of each laboratory data set includes error due to both the imprecision of the analytical method employed and to possible inhomogeneity of the material analysed. The standard deviation of the pooled individual analyses of all participating laboratories includes error due to the imprecision of each analytical method, to possible inhomogeneity of the material analysed and, in particular, to deficiencies in accuracy of each analytical method. In determining tolerance intervals that component of error attributable to measurement inaccuracy was eliminated by transformation of the individual results of each data set to a common mean (the uncorrected grand mean) according to the formula

$$x'_{ij} = x_{ij} - \bar{x}_i + \frac{\sum_{i=1}^p \sum_{j=1}^{n_i} x_{ij}}{\sum_{i=1}^p n_i}$$

where

x_{ij} is the j th raw result reported by laboratory i ;

x'_{ij} is the j th transformed result reported by laboratory i ;

n_i is the number of results reported by laboratory i ;

p is the number of participating laboratories;

\bar{x}_i is the raw mean for laboratory i .

The homogeneity of each constituent was determined from tables of factors for two-sided tolerance limits for normal distributions (ISO 3207) in which

$$\text{Lower limit is } \bar{x} - k'_2(n, p, 1 - \alpha) s_g''$$

$$\text{Upper limit is } \bar{x} + k'_2(n, p, 1 - \alpha) s_g''$$

where

n is the number of results;

$1 - \alpha$ is the confidence level;

p is the proportion of results expected within the tolerance limits;

k'_2 is the factor for two-sided tolerance limits (m, α unknown);

s_g'' is the corrected grand standard deviation.

The meaning of these tolerance limits may be illustrated for zinc by acid digest, where 99% of the time at least 95% of subsamples will have concentrations lying between 4.13 and 4.24 wt.%. Put more precisely, this means that if the same number of subsamples were taken and analysed in the same manner repeatedly, 99% of the tolerance intervals so constructed would cover at least 95% of the total population, and 1% of the tolerance intervals would cover less than 95% of the total population (ISO Guide 35).

The corrected grand standard deviation, s_g'' , used to compute the tolerance intervals is the weighted means of standard deviations of all data sets for a particular constituent according to the formula

$$s_g'' = \frac{\sum_{i=1}^p (s_i (1 - \frac{s_i}{s'_g}))}{\sum_{i=1}^p (1 - \frac{s_i}{s'_g})}$$

where

$$1 - (\frac{s_i}{s'_g}) \text{ is the weighting factor for laboratory } i;$$

s'_g is the grand standard deviation computed from the transformed (i.e. means-adjusted) results

according to the formula

$$s'_g = \left[\frac{\sum_{i=1}^p \sum_{j=i}^{n_i} (x'_{ij} - \bar{x}'_i)^2}{\sum_{i=1}^p n_i - 1} \right]^{1/2}$$

where \bar{x}'_i is the transformed mean for laboratory i

The weighting factors were applied to compensate for the considerable variation in analytical precision amongst participating laboratories. Hence, weighting factors for each data set have been constructed so as to be inversely proportional to the standard deviation of that data set. Individual outliers (shown in bold in Tables A2 to A18) were removed prior to the calculation of

tolerance intervals and a weighting factor of zero was applied to those data sets where $s_l / 2s_g' > 1$ (i.e. where the weighting factor $1 - s_l / 2s_g' < 0$). Data sets displaying poor resolution (i.e. where the ratio of the reading increment divided by the measured value is $< 1/20$) were also omitted.

It should be noted that estimates of tolerance by this method are considered conservative as a significant proportion of the observed variance, even in those laboratories exhibiting the best analytical precision, can presumably be attributed to measurement error. Despite the limitations of this method, the tolerance intervals presented in Table 2 are considered to confirm a high level of homogeneity for this CRM.

Table 2. Certified Values and Tolerance Limits for OREAS 36.

Constituent	Certified Value	Tolerance limits 1- α =0.99, ρ =0.95	
		Low	High
<u>Mixed Acid Digests (no HF)</u>			
Silver, Ag (ppm)	10.17	9.95	10.40
Arsenic, As (ppm)	722	705	739
Copper, Cu (ppm)	151	149	153
Iron, Fe (wt.%)	20.68	20.19	21.18
Manganese, Mn (wt.%)	1.08	1.06	1.10
Lead, Pb (wt.%)	0.579	0.569	0.588
Thallium, Tl (ppm)	~65	IND	IND
Zinc, Zn (wt.%)	4.19	4.13	4.24
<u>Peroxide Fusion</u>			
Silver, Ag (ppm)	9.6	IND	IND
Arsenic, As (ppm)	699	IND	IND
Copper, Cu (ppm)	153	IND	IND
Iron, Fe (wt.%)	21.06	20.68	21.44
Manganese, Mn (wt.%)	1.27	1.25	1.30
Lead, Pb (wt.%)	0.553	0.544	0.562
Thallium, Tl (ppm)	109	105	114
Zinc, Zn (wt.%)	4.22	4.13	4.32
<u>Leco</u>			
Sulphur, S (wt.%)	18.81	18.60	19.02

Note - intervals may appear asymmetric due to rounding

ANOVA Study

The sampling format for OREAS 36 was structured to enable nested ANOVA treatment of the round robin results. During the bagging stage immediately following final homogenization, samples were taken at 10 intervals representative of the entire batch of OREAS 36. Each lab received 4 samples per batch made up of paired samples from two different (non-adjacent) intervals. For example, the four samples that Lab A received consisted of:

- Sample 1 (from sampling interval 1)
- Sample 2 (from sampling interval 6)
- Sample 3 (from sampling interval 1)
- Sample 4 (from sampling interval 6)

The acid digest zinc results were used as the test data for the ANOVA investigation comparing within- and between-unit variance. This approach permitted an assessment of homogeneity across the entire batch of OREAS 36. The test was performed using the following parameters:

- Significance Level $\alpha = P$ (type I error) = 0.05
- Null Hypothesis, H_0 : Between-unit variance is no greater than within-unit variance (reject H_0 if p-value < 0.05)
- Alternative Hypothesis, H_1 : Between-unit variance is greater than within-unit variance

P-values are a measure of probability whereby values less than 0.05 indicate a greater than 95% probability that the observed differences in within-unit and between-unit variances are real. The same filtered dataset used to calculate the certified value for zinc via acid digest was used yielding a total of 76 samples from nine labs. The derived p-value of 0.9990 indicates no evidence that between-unit variance is greater than within-unit variance. Conclusion: do not reject H_0 . Note that ANOVA is not an absolute measure of homogeneity. Rather, it establishes that zinc is uniformly distributed throughout OREAS 36 and that the variance between two aliquots from the same unit is identical to the variance from two aliquots taken from any two separate units.

Performance Gates

Performance gates provide an indication of a level of performance that might reasonably be expected from a laboratory being monitored by this standard in a QA/QC program. They take into account errors attributable to measurement and CRM variability. For an effective CRM the contribution of the latter should be negligible in comparison to measurement errors. Sources of measurement error include inter-lab bias, analytical precision (repeatability) and inter-batch bias (reproducibility).

Performance gates have been calculated from the same filtered data set used to determine the certified value, i.e. after removal of all individual and batch outliers. These outliers can only be removed after the absolute homogeneity of the CRM has been independently established, i.e. the outliers must be confidently deemed to be analytical rather than arising from inhomogeneity of the CRM. The standard deviations are then calculated for each lab's results and then each SD is tested for outlying status using z-score discrimination (rejected if $|z_i| > 2.5$). The 1SD used to calculate performance gates is the mean of the remaining (accepted) lab standard deviations. Because batch to batch bias is an important component of performance gates, only results from the six labs that received 3 submissions of samples have been used in the calculations.

Table 3 shows performance gates calculated for two and three standard deviations. As a guide these intervals may be regarded as warning or rejection for multiple 2SD outliers, or rejection for individual 3SD outliers in QC monitoring, although their precise application should be at the discretion of the QC manager concerned. Standard deviation is also shown in relative percent for one, two and three relative standard deviations (1RSD, 2RSD and 3RSD) to facilitate comparison with a 5% window calculated directly from the certified value. Caution should be exercised when concentration levels approach lower limits of detection of the analytical methods employed as performance gates calculated from standard deviations tend to be excessively wide whereas those determined by the 5% method are too narrow.

Table 3. Performance Gates for OREAS 36.

Constituent	Certified Value	5% window		Relative Standard Deviations			1SD	2SD window		3SD window	
		Low	High	1RSD	2RSD	3RSD		Low	High	Low	High
Mixed Acid Digests (no HF)											
Ag (ppm)	10.17	9.67	10.68	6.23%	12.5%	18.7%	0.63	8.91	11.44	8.27	12.08
As (ppm)	722	686	758	4.45%	8.90%	13.3%	32	658	786	626	819
Cu (ppm)	151	143	158	3.00%	6.00%	8.99%	5	142	160	137	165
Fe (wt.%)	20.68	19.65	21.72	1.80%	3.60%	5.40%	0.37	19.94	21.43	19.57	21.80
Mn (wt.%)	1.08	1.03	1.13	3.11%	6.22%	9.32%	0.03	1.01	1.15	0.98	1.18
Pb (wt.%)	0.579	0.550	0.608	2.84%	5.68%	8.51%	0.016	0.546	0.611	0.529	0.628
Tl (ppm)	~65	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
Zn (wt.%)	4.19	3.98	4.39	1.61%	3.22%	4.83%	0.07	4.05	4.32	3.98	4.39
Peroxide Fusion											
Ag (ppm)	~9.6	IND	IND	IND	IND	IND	IND	IND	IND	IND	IND
As (ppm)	699	664	733	7.71%	15.4%	23.1%	54	591	806	537	860
Cu (ppm)	153	145	160	4.42%	8.84%	13.3%	7	139	166	132	173
Fe (wt.%)	21.06	20.01	22.11	4.01%	8.03%	12.0%	0.85	19.37	22.75	18.52	23.60
Mn (wt.%)	1.27	1.21	1.34	2.67%	5.33%	8.00%	0.03	1.20	1.34	1.17	1.37
Pb (wt.%)	0.553	0.525	0.580	2.14%	4.29%	6.43%	0.01	0.529	0.576	0.517	0.588
Tl (ppm)	109	104	115	2.71%	5.42%	8.13%	3	103	115	100	118
Zn (wt.%)	4.22	4.01	4.43	3.15%	6.31%	9.46%	0.13	3.96	4.49	3.82	4.62
Leco											
S (wt.%)	18.81	17.87	19.75	1.15%	2.29%	3.44%	0.22	18.38	19.24	18.16	19.45

Note - intervals may appear asymmetric due to rounding

PARTICIPATING LABORATORIES

Acme Analytical Laboratories, Vancouver, BC, Canada
 Activation Laboratories, Ancaster, Ontario, Canada
 ALS Chemex, Johannesburg, Australia
 ALS Chemex, Stafford, QLD, Australia
 ALS Chemex, North Vancouver, BC, Canada
 Amdel Laboratories, Perth, WA, Australia
 Genalysis, Maddington, WA, Australia
 SGS Analabs, Welshpool, Perth, WA, Australia
 OMAC, Loughrea, Ireland
 Ultra Trace, Canning Vale, WA, Australia

PREPARER AND SUPPLIER OF THE REFERENCE MATERIAL

The reference material OREAS 36 has been prepared and certified by:

Ore Research & Exploration Pty Ltd
 6-8 Gatwick Road
 Bayswater North VIC 3153
 AUSTRALIA

Telephone	(03) 9729 0333	International	+613-9729 0333
Facsimile	(03) 9729 4777	International	+613-9729 4777
Email	info@ore.com.au	Web	www.ore.com.au

OREAS 36 has been packaged under nitrogen in laminated foil pouches in 10g units.

INTENDED USE

OREAS 36 is a reference material intended for the following:

- i) for the calibration of instruments used in the determination of the concentration of Ag, As, Cu, Fe, Mn, Pb, S, Tl and Zn;
- ii) for the verification of analytical methods for Ag, As, Cu, Fe, Mn, Pb, S, Tl and Zn;
- iii) for the monitoring of laboratory performance in the analysis of Ag, As, Cu, Fe, Mn, Pb, S, Tl and Zn in geological samples.

STABILITY AND STORAGE INSTRUCTIONS

OREAS 36 is sourced from low grade zinc sulphide ore and has been packaged under dry nitrogen in robust laminated foil pouches. In its unopened state and under normal conditions of storage it has a shelf life beyond five years.

INSTRUCTIONS FOR THE CORRECT USE OF THE REFERENCE MATERIAL

The certified values for CRM OREAS 36 refer to the concentration level of Ag, As, Cu, Fe, Mn, Pb, S, Tl and Zn in its packaged state. Therefore it should not be dried prior to weighing and analysis.

LEGAL NOTICE

Ore Research & Exploration Pty Ltd has prepared and statistically evaluated the property values of this reference material to the best of its ability. The Purchaser by receipt hereof releases and indemnifies Ore Research & Exploration Pty Ltd from and against all liability and costs arising from the use of this material and information.

CERTIFYING OFFICER:

Dr Paul Hamlyn

REFERENCES

- ISO Guide 35 (2006), Certification of reference materials - General and statistical principals.
- ISO Guide 3207 (1975), Statistical interpretation of data - Determination of a statistical tolerance interval.
- Rozendaal, A. & Stalder, M. 2001. REE geochemistry of garnet associated with the Gamsberg Zn-Pb deposit, South Africa. *Mineral Deposits at the Beginning of the 21st Century*, pp. 325.

APPENDIX

Analytical Data for OREAS 36

Table A1. Key to abbreviations used in Tables A2 – A18.

Abbreviation	Explanation
Std.Dev.	one sigma standard deviation
Rel.Std.Dev.	one sigma relative standard deviation
PDM ³	percent deviation of lab mean from corrected mean of means
PF	sodium peroxide fusion
AR	aqua regia digest (HNO ₃ -HCl)
3A	three acid digest (HNO ₃ -HCl-HClO ₄)
MA	mixed acid digest (KClO ₄ -HNO ₃ -HBr-HCl)
OES	inductively coupled plasma optical emission spectrometry
MS	inductively coupled plasma mass spectrometry
AAS	atomic absorption spectrometry
Leco	IR combustion furnace

Table A2. Mixed acid digest (no HF) results for Ag in OREAS 36 (abbreviations as in Table A1; values in ppm)

Replicate No.	Lab A 3A*MS	Lab B 3A*OES	Lab C AR*MS	Lab D AR*OES	Lab E AR*OES	Lab F MA*MS	Lab G AR*OES	Lab H 3A*MS	Lab I 3A*MS	Lab J AR*OES
1	9.50	10.00	9.90	11.00	12.00	9.74	10.00	10.00	10.00	10.00
2	9.80	11.00	9.70	10.00	10.00	10.02	10.00	10.00	9.00	11.00
3	9.80	10.00	9.70	11.00	11.00	9.89	11.00	10.00	9.00	13.00
4	9.70	9.00	9.60	11.00	10.00	9.95	10.00	10.00	9.00	14.00
5	11.00	9.00	8.87	11.00	8.00	10.05				
6	11.00	11.00	8.65	11.00	9.00	10.04				
7	10.00	10.00	8.22	10.00	9.00	9.70				
8	11.00	12.00	7.82	10.00	9.00	9.97				
9	9.60	11.00	10.00	10.00	8.00	10.15				
10	10.00	12.00	9.90	10.00	9.00	10.28				
11	9.60	12.00	9.90	10.00	8.00	10.13				
12	9.70	11.00	9.90	11.00	8.00	10.34				
Mean	10.06	10.67	9.35	10.50	9.25	10.02	10.25	10.00	9.25	12.00
Median	9.80	11.00	9.70	10.50	9.00	10.03	10.00	10.00	9.00	12.00
Std.Dev.	0.59	1.07	0.76	0.52	1.29	0.19	0.50	0.00	0.50	1.83
Rel.Std.Dev.	5.84%	10.1%	8.08%	4.97%	13.9%	1.91%	4.88%	0.00%	5.41%	15.2%
PDM ³	-1.14%	4.84%	-8.14%	3.20%	-9.09%	-1.50%	0.74%	-1.72%	-9.09%	17.9%

Table A3. Mixed acid digest (no HF) results for As in OREAS 36 (abbreviations as in Table A1; values in ppm)

Replicate No.	Lab A 3A*MS	Lab B 3A*OES	Lab C AR*MS	Lab D AR*OES	Lab E AR*OES	Lab F MA*MS	Lab G AR*OES	Lab H 3A*MS	Lab I 3A*MS	Lab J AR*OES
1	721	700	NR	720	780	745	630	760	742	720
2	768	700	NR	730	720	762	630	752	706	740
3	761	700	NR	720	670	744	640	767	731	730
4	748	700	NR	720	740	760	640	737	680	740
5	712	700	754	730	720	748				
6	727	700	740	720	810	751				
7	726	700	658	680	660	752				
8	695	800	723	710	700	746				
9	679	700	654	730	670	735				
10	664	700	643	760	780	738				
11	664	700	651	750	670	738				
12	672	700	648	740	670	736				
Mean	711	708	684	726	716	746	635	754	715	733
Median	717	700	656	725	710	746	635	756	719	735
Std.Dev.	37	29	47	20	52	9	6	13	28	10
Rel.Std.Dev.	5.18%	4.08%	6.81%	2.78%	7.23%	1.20%	0.91%	1.71%	3.87%	1.31%
PDM ³	-1.49%	-1.92%	-5.31%	0.50%	-0.88%	3.33%	-12.1%	4.40%	-1.03%	1.43%

Table A4. Mixed acid digest (no HF) results for Cu in OREAS 36 (abbreviations as in Table A1; values in ppm)

Replicate No.	Lab A	Lab B	Lab C	Lab D	Lab E	Lab F	Lab G	Lab H	Lab I	Lab J
	3A*MS	3A*OES	AR*OES	AR*OES	AR*OES	MA*MS	AR*OES	3A*OES	3A*OES	AR*OES
1	144	140	130	144	131	152	150	163	145	150
2	148	140	130	142	130	155	150	157	150	154
3	148	140	130	143	135	151	200	163	150	155
4	145	140	130	144	130	152	150	157	150	150
5	159	140	137	150	137	151				
6	162	140	132	150	144	151				
7	166	150	128	156	141	150				
8	156	150	158	146	147	150				
9	150	140	157	149	153	155				
10	151	140	154	150	159	157				
11	149	140	159	151	152	154				
12	146	140	155	154	146	155				
Mean	152	142	142	148	142	153	163	160	149	152
Median	150	140	135	150	143	152	150	160	150	152
Std.Dev.	7	4	13	4	10	2	25	3	3	3
Rel.Std.Dev.	4.68%	2.75%	9.47%	3.00%	6.84%	1.57%	15.38%	2.17%	1.68%	1.73%
PDM ³	0.71%	-6.14%	-6.14%	-1.78%	-5.86%	1.24%	7.66%	6.01%	-1.45%	0.87%

Table A5. Mixed acid digest (no HF) results for Fe in OREAS 36 (abbreviations as in Table A1; values in wt.%)

Replicate No.	Lab A	Lab B	Lab C	Lab D	Lab E	Lab F	Lab G	Lab H	Lab I	Lab J
	3A*OES	3A*OES	AR*OES	AR*OES	AR*OES	MA*MS	AR*OES	3A*OES	3A*OES	AR*OES
1	20.50	19.96	15.10	19.90	20.20	19.39	20.57	21.45	21.90	20.70
2	20.70	20.07	16.30	20.00	20.10	19.57	20.42	21.58	22.30	20.90
3	21.10	19.86	15.80	20.40	20.60	19.56	20.85	21.93	21.10	20.80
4	20.70	19.29	16.20	19.95	20.10	19.76	20.44	21.49	21.20	20.60
5	21.50	20.63	18.00	21.00	20.30	19.96				
6	22.10	20.85	18.70	21.30	20.70	19.95				
7	21.80	20.95	18.50	20.50	20.30	20.07				
8	21.40	21.71	17.90	20.70	21.30	20.02				
9	20.70	20.34	19.90	20.90	20.10	19.85				
10	21.50	20.74	19.90	21.20	21.10	19.89				
11	20.80	20.83	20.60	21.30	20.90	19.83				
12	21.10	20.60	19.70	21.70	20.20	20.04				
Mean	21.16	20.49	18.05	20.74	20.49	19.82	20.57	21.61	21.63	20.75
Median	21.10	20.62	18.25	20.80	20.30	19.87	20.51	21.54	21.55	20.75
Std.Dev.	0.50	0.63	1.83	0.60	0.42	0.21	0.20	0.22	0.57	0.13
Rel.Std.Dev.	2.38%	3.07%	10.2%	2.87%	2.05%	1.08%	0.96%	1.01%	2.65%	0.62%
PDM ³	2.30%	-0.95%	-12.7%	0.26%	-0.93%	-4.15%	-0.55%	4.49%	4.55%	0.32%

Table A6. Mixed acid digest (no HF) results for Mn in OREAS 36 (abbreviations as in Table A1; values in wt.%)

Replicate No.	Lab A 3A*AAS	Lab B 3A*OES	Lab C AR*OES	Lab D AR*OES	Lab E AR*OES	Lab F MA*MS	Lab G AR*OES	Lab H 3A*OES	Lab I 3A*OES	Lab J AR*OES
1	1.21	1.11	0.85	0.91	0.80	0.95	1.34	1.16	1.07	1.02
2	1.25	1.10	0.91	0.92	0.80	0.96	1.26	1.15	1.14	1.02
3	1.25	1.11	0.87	0.94	0.81	0.99	1.38	1.19	1.11	1.02
4	1.24	1.09	0.91	0.92	0.79	0.97	1.31	1.16	1.06	1.02
5	1.28	1.10	1.15	0.91	0.92	0.98				
6	1.22	1.16	1.04	0.91	0.95	0.97				
7	1.24	1.17	1.00	0.88	0.93	0.96				
8	1.23	1.16	0.98	0.89	0.98	0.97				
9	1.30	1.14	1.22	0.96	0.85	0.96				
10	1.29	1.16	1.26	0.97	0.89	0.97				
11	1.24	1.15	1.17	0.98	0.89	0.99				
12	1.26	1.15	1.22	1.00	0.86	0.99				
Mean	1.25	1.13	1.05	0.93	0.87	0.97	1.32	1.16	1.10	1.02
Median	1.25	1.15	1.02	0.92	0.87	0.97	1.32	1.16	1.09	1.02
Std.Dev.	0.03	0.03	0.15	0.04	0.06	0.01	0.05	0.02	0.04	0.00
Rel.Std.Dev.	2.19%	2.56%	14.3%	4.03%	7.38%	1.26%	3.86%	1.37%	3.38%	0.25%
PDM ³	15.8%	4.95%	-2.95%	-13.7%	-19.4%	-9.77%	22.3%	7.60%	1.40%	-5.66%

Table A7. Mixed acid digest (no HF) results for Pb in OREAS 36 (abbreviations as in Table A1; values in wt.%)

Replicate No.	Lab A 3A*AAS	Lab B 3A*OES	Lab C AR*OES	Lab D AR*OES	Lab E AR*OES	Lab F MA*MS	Lab G AR*OES	Lab H 3A*MS	Lab I 3A*MS	Lab J AR*OES
1	0.487	0.580	0.605	0.557	0.570	0.603	0.575	0.560	0.548	0.598
2	0.486	0.580	0.616	0.559	0.590	0.616	0.590	0.556	0.568	0.601
3	0.499	0.590	0.602	0.564	0.610	0.602	0.595	0.554	0.563	0.598
4	0.516	0.570	0.606	0.556	0.600	0.615	0.580	0.549	0.541	0.596
5	0.550	0.590	0.582	0.569	0.578	0.587				
6	0.540	0.620	0.586	0.587	0.566	0.592				
7	0.530	0.620	0.587	0.555	0.560	0.593				
8	0.540	0.640	0.588	0.566	0.592	0.596				
9	0.577	0.610	0.590	0.581	0.533	0.600				
10	0.606	0.620	0.579	0.585	0.572	0.598				
11	0.568	0.620	0.576	0.587	0.552	0.601				
12	0.573	0.600	0.580	0.595	0.545	0.598				
Mean	0.539	0.603	0.591	0.572	0.572	0.600	0.585	0.555	0.555	0.598
Median	0.540	0.605	0.588	0.568	0.571	0.599	0.585	0.555	0.556	0.598
Std.Dev.	0.038	0.021	0.013	0.014	0.023	0.008	0.009	0.005	0.013	0.002
Rel.Std.Dev.	7.02%	3.56%	2.16%	2.52%	4.02%	1.39%	1.56%	0.86%	2.27%	0.34%
PDM ³	-6.78%	4.28%	2.22%	-1.18%	-1.08%	3.71%	1.11%	-4.14%	-4.07%	3.40%

Table A8. Mixed acid digest (no HF) results for TI in OREAS 36 (abbreviations as in Table A1; values in ppm)

Replicate No.	Lab A 3A*MS	Lab B 3A*OES	Lab C AR*OES	Lab D AR*OES	Lab E AR*OES	Lab F MA*MS	Lab G AR*OES	Lab H 3A*MS	Lab I 3A*MS	Lab J AR*OES
1	99	100	52	<50	<50	24	50	115	44	50
2	104	100	53	<50	<50	29	50	116	47	50
3	103	100	55	<50	<50	31	70	118	43	<50
4	101	100	53	<50	<50	32	60	114	41	<50
5	99	100	43	50	<50	22				
6	102	100	44	50	<50	24				
7	103	100	42	<50	60	26				
8	102	100	51	<50	<50	28				
9	82	NR	56	50	50	23				
10	97	NR	58	<50	<50	25				
11	93	NR	56	<50	50	26				
12	100	NR	57	<50	<50	28				
Mean	99	100	52	50	53	27	58	116	44	50
Median	100	100	53	50	50	26	55	115	44	50
Std.Dev.	6	0	6	0	6	3	10	1	3	0
Rel.Std.Dev.	6.17%	0.00%	10.9%	0.00%	10.8%	11.6%	16.7%	1.28%	5.71%	0.00%
PDM ³	52.8%	54.9%	-20.0%	-22.6%	-17.4%	-58.9%	-11.0%	79.1%	-32.2%	-22.6%

Table A9. Mixed acid digest (no HF) results for Zn in OREAS 36 (abbreviations as in Table A1; values in wt.%)

Replicate No.	Lab A 3A*AAS	Lab B 3A*OES	Lab C AR*OES	Lab D AR*OES	Lab E AR*OES	Lab F MA*MS	Lab G AR*OES	Lab H 3A*OES	Lab I 3A*OES	Lab J AR*OES
1	4.18	4.22	4.18	4.03	4.15	4.15	4.26	4.16	4.51	4.17
2	4.07	4.27	4.12	4.00	4.24	4.18	4.24	4.19	4.52	4.24
3	4.13	4.25	4.03	4.09	4.41	4.13	4.32	4.27	4.46	4.22
4	4.11	4.12	4.01	4.02	4.34	4.19	4.24	4.16	4.32	4.20
5	4.05	4.21	3.98	4.16	4.02	4.13				
6	4.05	4.38	4.07	4.25	4.25	4.17				
7	3.90	4.32	3.98	4.09	4.32	4.16				
8	4.03	4.44	4.01	4.09	4.37	4.16				
9	3.89	4.48	4.01	4.20	4.30	4.17				
10	4.05	4.51	4.04	4.23	4.38	4.20				
11	4.02	4.61	3.97	4.24	4.40	4.16				
12	4.08	4.57	3.96	4.33	4.46	4.15				
Mean	4.05	4.37	4.03	4.14	4.30	4.16	4.27	4.20	4.45	4.21
Median	4.05	4.35	4.01	4.13	4.33	4.16	4.25	4.17	4.49	4.21
Std.Dev.	0.08	0.16	0.07	0.11	0.12	0.02	0.04	0.05	0.09	0.03
Rel.Std.Dev.	2.07%	3.60%	1.6%	2.56%	2.87%	0.50%	0.89%	1.29%	2.07%	0.71%
PDM ³	-3.31%	4.30%	-3.71%	-0.98%	2.82%	-0.51%	1.91%	0.23%	6.39%	0.53%

Table A10. Peroxide fusion results for Ag in OREAS 36 (abbreviations as in Table A1; values in ppm)

Replicate No.	Lab A PF*MS	Lab B -	Lab C PF*OES	Lab D -	Lab E -	Lab F -	Lab G PF*OES	Lab H PF*MS	Lab I PF*MS	Lab J PF*OES
1	10.00	NR	< 60	NR	NR	NR	<20	8.00	10.00	NR
2	10.00	NR	< 60	NR	NR	NR	<20	8.00	10.00	NR
3	10.00	NR	< 60	NR	NR	NR	<20	9.00	10.00	NR
4	10.00	NR	< 60	NR	NR	NR	<20	9.00	10.00	NR
5	11.00	NR	9.90	NR	NR	NR				
6	11.00	NR	9.80	NR	NR	NR				
7	11.00	NR	9.50	NR	NR	NR				
8	11.00	NR	9.60	NR	NR	NR				
9	10.00	NR	< 50	NR	NR	NR				
10	10.00	NR	< 50	NR	NR	NR				
11	10.00	NR	< 50	NR	NR	NR				
12	10.00	NR	< 50	NR	NR	NR				
Mean	10.33		9.70					8.50	10.00	
Median	10.00		9.70					8.50	10.00	
Std.Dev.	0.49		0.18					0.58	0.00	
Rel.Std.Dev.	4.76%		1.88%					6.79%	0.00%	
PDM ³	7.27%		0.69%					-11.8%	3.81%	

Table A11. Peroxide fusion results for As in OREAS 36 (abbreviations as in Table A1; values in ppm)

Replicate No.	Lab A PF*MS	Lab B PF*OES	Lab C PF*OES	Lab D PF*OES	Lab E -	Lab F -	Lab G PF*OES	Lab H PF*MS	Lab I PF*MS	Lab J PF*OES
1	700	600	600	800	NR	NR	660	773	780	900
2	750	600	500	700	NR	NR	730	803	810	1000
3	750	600	600	700	NR	NR	670	874	795	900
4	750	600	500	700	NR	NR	645	799	820	800
5	650	700	600	700	NR	NR				
6	670	700	600	800	NR	NR				
7	650	700	700	600	NR	NR				
8	680	700	600	700	NR	NR				
9	640	NR	600	700	NR	NR				
10	650	NR	700	600	NR	NR				
11	680	NR	600	700	NR	NR				
12	690	NR	600	700	NR	NR				
Mean	688	650	600	700			676	812	801	900
Median	680	650	600	700			665	801	803	900
Std.Dev.	41	53	60	60			37	43	18	82
Rel.Std.Dev.	6.00%	8.22%	10.1%	8.61%			5.51%	5.33%	2.18%	9.07%
PDM ³	-1.46%	-6.95%	-14.1%	0.21%			-3.19%	16.3%	14.7%	28.8%

Table A12. Peroxide fusion results for Cu in OREAS 36 (abbreviations as in Table A1; values in ppm)

Replicate No.	Lab A PF*MS	Lab B PF*OES	Lab C PF*OES	Lab D PF*OES	Lab E -	Lab F -	Lab G PF*OES	Lab H PF*OES	Lab I PF*OES	Lab J PF*OES
1	170	180	150	160	NR	NR	145	NR	140	200
2	190	170	150	160	NR	NR	170	NR	160	200
3	170	160	150	210	NR	NR	155	700	150	200
4	160	160	150	150	NR	NR	245	NR	160	200
5	140	150	150	160	NR	NR				
6	150	150	150	160	NR	NR				
7	160	150	150	160	NR	NR				
8	150	150	150	140	NR	NR				
9	150	100	130	150	NR	NR				
10	150	100	160	160	NR	NR				
11	160	100	130	150	NR	NR				
12	150	100	140	190	NR	NR				
Mean	158	139	147	163			179	700	153	200
Median	155	150	150	160			163	700	155	200
Std.Dev.	13	30	9	19			45		10	0
Rel.Std.Dev.	8.44%	21.8%	6.05%	11.8%			25.4%		6.28%	0.00%
PDM ³	3.78%	-8.78%	-3.87%	6.51%			17.2%	359%	-0.05%	31.1%

Table A13. Peroxide fusion results for Fe in OREAS 36 (abbreviations as in Table A1; values in wt.%)

Replicate No.	Lab A PF*OES	Lab B PF*OES	Lab C PF*OES	Lab D PF*OES	Lab E -	Lab F -	Lab G PF*OES	Lab H PF*OES	Lab I PF*OES	Lab J PF*OES
1	22.10	19.28	20.70	21.40	NR	NR	20.10	21.44	22.30	30.90
2	22.70	18.62	20.60	20.80	NR	NR	20.50	21.75	22.50	30.70
3	22.00	19.35	20.20	20.10	NR	NR	20.20	21.60	22.65	30.30
4	20.40	19.35	20.60	20.50	NR	NR	20.00	20.93	22.10	29.10
5	21.00	20.67	21.10	21.90	NR	NR				
6	21.90	20.38	21.30	22.00	NR	NR				
7	21.50	20.70	21.40	21.20	NR	NR				
8	21.70	20.81	20.90	20.80	NR	NR				
9	21.10	20.90	21.30	19.65	NR	NR				
10	19.20	20.53	21.10	19.95	NR	NR				
11	20.80	20.73	20.70	19.80	NR	NR				
12	20.30	21.08	20.80	19.60	NR	NR				
Mean	21.23	20.20	20.89	20.64			20.20	21.43	22.39	30.25
Median	21.30	20.60	20.85	20.65			20.15	21.52	22.40	30.50
Std.Dev.	0.96	0.82	0.36	0.85			0.22	0.36	0.24	0.81
Rel.Std.Dev.	4.53%	4.04%	1.71%	4.11%			1.07%	1.66%	1.07%	2.67%
PDM ³	0.78%	-4.08%	-0.80%	-1.99%			-4.08%	1.76%	6.30%	43.6%

Table A14. Peroxide fusion results for Mn in OREAS 36 (abbreviations as in Table A1; values in wt.%)

Replicate No.	Lab A PF*OES	Lab B PF*OES	Lab C PF*OES	Lab D PF*OES	Lab E -	Lab F -	Lab G PF*OES	Lab H PF*OES	Lab I PF*OES	Lab J PF*OES
1	1.29	1.19	1.24	1.39	NR	NR	1.67	1.30	1.28	1.30
2	1.33	1.19	1.24	1.35	NR	NR	1.71	1.30	1.26	1.30
3	1.29	1.22	1.24	1.30	NR	NR	1.68	1.30	1.28	1.28
4	1.19	1.24	1.23	1.32	NR	NR	1.65	1.30	1.28	1.22
5	1.47	1.23	1.25	1.34	NR	NR				
6	1.53	1.21	1.25	1.35	NR	NR				
7	1.51	1.26	1.26	1.30	NR	NR				
8	1.53	1.24	1.24	1.27	NR	NR				
9	1.30	NR	1.25	1.23	NR	NR				
10	1.18	NR	1.24	1.25	NR	NR				
11	1.29	NR	1.22	1.25	NR	NR				
12	1.25	NR	1.23	1.23	NR	NR				
Mean	1.35	1.22	1.24	1.30			1.68	1.30	1.28	1.28
Median	1.30	1.23	1.24	1.30			1.68	1.30	1.28	1.29
Std.Dev.	0.13	0.02	0.01	0.05			0.03	0.00	0.01	0.04
Rel.Std.Dev.	9.57%	2.04%	0.87%	3.98%			1.49%	0.00%	0.78%	2.86%
PDM ³	5.85%	-3.91%	-2.47%	2.06%			31.9%	2.18%	0.21%	0.29%

Table A15. Peroxide fusion results for Pb in OREAS 36 (abbreviations as in Table A1; values in wt.%)

Replicate No.	Lab A PF*MS	Lab B PF*OES	Lab C PF*OES	Lab D PF*OES	Lab E -	Lab F -	Lab G -	Lab H PF*MS	Lab I PF*MS	Lab J PF*OES
1	0.537	0.530	0.560	0.590	NR	NR	NR	0.559	0.574	0.560
2	0.542	0.530	0.550	0.550	NR	NR	NR	0.532	0.583	0.540
3	0.559	0.540	0.560	0.540	NR	NR	NR	0.565	0.575	0.540
4	0.554	0.560	0.550	0.560	NR	NR	NR	0.560	0.572	0.500
5	0.476	0.610	0.550	0.590	NR	NR				
6	0.517	0.600	0.550	0.600	NR	NR				
7	0.516	0.610	0.550	0.560	NR	NR				
8	0.509	0.620	0.550	0.560	NR	NR				
9	0.542	NR	0.560	0.550	NR	NR				
10	0.514	NR	0.560	0.550	NR	NR				
11	0.531	NR	0.540	0.550	NR	NR				
12	0.544	NR	0.550	0.530	NR	NR				
Mean	0.528	0.575	0.553	0.561				0.554	0.576	0.535
Median	0.534	0.580	0.550	0.555				0.560	0.574	0.540
Std.Dev.	0.023	0.039	0.006	0.022				0.015	0.005	0.025
Rel.Std.Dev.	4.38%	6.77%	1.13%	3.84%				2.69%	0.85%	4.70%
PDM ³	-4.39%	4.04%	-0.03%	1.48%				0.27%	4.20%	-3.20%

Table A16. Peroxide fusion results for TI in OREAS 36 (abbreviations as in Table A1; values in ppm)

Replicate No.	Lab A PF*MS	Lab B PF*OES	Lab C PF*OES	Lab D -	Lab E -	Lab F -	Lab G -	Lab H PF*MS	Lab I PF*MS	Lab J -
1	101	100	137	NR	NR	NR	NR	111	113	NR
2	106	100	139	NR	NR	NR	NR	111	106	NR
3	106	100	138	NR	NR	NR	NR	113	106	NR
4	103	100	136	NR	NR	NR	NR	116	110	NR
5	98	100	124	NR	NR	NR				
6	102	100	127	NR	NR	NR				
7	100	100	127	NR	NR	NR				
8	97	100	121	NR	NR	NR				
9	104	NR	119	NR	NR	NR				
10	98	NR	125	NR	NR	NR				
11	99	NR	123	NR	NR	NR				
12	100	NR	127	NR	NR	NR				
Mean	101	100	129					113	109	
Median	101	100	127					112	108	
Std.Dev.	3	0	7					2	3	
Rel.Std.Dev.	2.93%	0.00%	5.47%					2.11%	3.13%	
PDM ³	-7.27%	-8.42%	17.8%					3.26%	-0.41%	

Table A17. Peroxide fusion results for Zn in OREAS 36 (abbreviations as in Table A1; values in wt.%)

Replicate No.	Lab A PF*OES	Lab B PF*OES	Lab C PF*OES	Lab D PF*OES	Lab E -	Lab F -	Lab G PF*OES	Lab H PF*OES	Lab I PF*OES	Lab J PF*OES
1	4.13	4.18	4.04	4.35	NR	NR	2.84	4.18	4.53	4.10
2	4.25	4.22	4.03	4.25	NR	NR	2.89	4.19	4.51	4.11
3	4.02	4.20	4.07	4.00	NR	NR	2.87	4.43	4.46	4.08
4	3.97	4.38	3.95	4.09	NR	NR	2.78	4.07	4.41	3.93
5	4.19	4.44	3.89	4.25	NR	NR				
6	4.38	4.42	3.93	4.41	NR	NR				
7	4.32	4.56	3.97	4.22	NR	NR				
8	4.33	4.51	3.91	4.04	NR	NR				
9	4.27	4.54	4.28	4.13	NR	NR				
10	4.09	4.50	4.25	4.19	NR	NR				
11	4.29	4.38	4.13	4.15	NR	NR				
12	4.15	4.43	4.18	4.07	NR	NR				
Mean	4.20	4.40	4.05	4.18			2.85	4.22	4.48	4.06
Median	4.22	4.43	4.04	4.17			2.86	4.19	4.48	4.09
Std.Dev.	0.13	0.13	0.13	0.12			0.05	0.15	0.05	0.08
Rel.Std.Dev.	3.08%	3.00%	3.27%	2.96%			1.69%	3.60%	1.21%	2.08%
PDM ³	-0.56%	4.12%	-4.03%	-1.03%			-32.6%	-0.12%	6.00%	-3.97%

Table A18. Results for S in OREAS 36 (abbreviations as in Table A1; values in wt.%)

Replicate No.	Lab A Leco	Lab B Leco	Lab C Leco	Lab D Leco	Lab E Leco	Lab F Leco	Lab G AR*OES	Lab H Leco	Lab I Leco	Lab J Leco
1	19.40	18.41	17.00	18.35	18.40	19.68	18.85	19.37	18.70	18.30
2	19.80	19.59	17.60	18.10	18.60	19.59	19.10	19.88	19.00	18.50
3	18.70	18.69	18.10	17.60	18.40	19.85	19.35	19.95	18.80	18.40
4	19.30	18.40	18.10	18.45	18.30	20.07	18.75	19.50	18.80	18.60
5	19.10	18.27	19.00	18.60	17.90	19.60				
6	19.20	19.00	18.70	18.95	17.90	19.68				
7	19.30	18.35	18.90	18.60	17.30	19.49				
8	19.10	18.01	19.20	18.65	18.10	19.44				
9	19.30	NR	17.80	17.50	18.20	19.85				
10	19.40	NR	18.70	17.45	18.30	19.82				
11	19.30	NR	19.00	18.80	18.40	19.89				
12	19.40	NR	19.10	17.85	19.10	19.71				
Mean	19.28	18.59	18.43	18.24	18.24	19.72	19.01	19.67	18.83	18.45
Median	19.30	18.41	18.70	18.40	18.30	19.69	18.98	19.69	18.80	18.45
Std.Dev.	0.26	0.50	0.70	0.53	0.44	0.18	0.27	0.28	0.13	0.13
Rel.Std.Dev.	1.33%	2.68%	3.80%	2.89%	2.39%	0.92%	1.41%	1.43%	0.67%	0.70%
PDM ³	2.49%	-1.15%	-1.99%	-3.01%	-3.01%	4.86%	1.09%	4.61%	0.09%	-1.90%